
Introducing NUVETEST[™] – Fast, accurate and convenient.

A one-step detection test for vaginitis associated with bacterial vaginosis (BV) and trichomonas.



NUVETEST™ effectively measures vaginal acidity associated with BV due to its buffer capacity

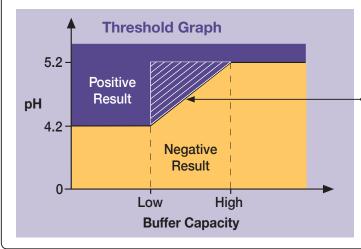

The inclusion of buffer capacity allows NUVETEST[™] to capture those patients misdiagnosed with pH paper alone.

 Unlike regular pH tests which miss about 22% of BV cases with normal pH levels, NUVETEST[™] improves detection accuracy to approximately 90% for added assurance.¹

Interpretation of NUVETESTTM results

Positive Result

 If the tip of the NUVETEST[™] swab is stained or partially stained blue or green, vaginal acidity is disordered and infections associated with high pH are quite probable.

> Additional testing for bacterial vaginosis (BV) and trichomonas should be considered.

Negative Result


- If after **10 seconds** the NUVETEST[™] tip is not stained, ie, completely yellow, vaginal acidity is normal.
 - The risk of having an infection associated with elevated pH levels is unlikely.

NUVETEST[™]

Important: If the patient is pregnant and the tip of the NUVETESTTMswab is stained blue or green, the color change may indicate an amniotic fluid leak.

Please see Warnings and Precautions on reverse side.

Introducing NUVETESTTM – now available in full supply!

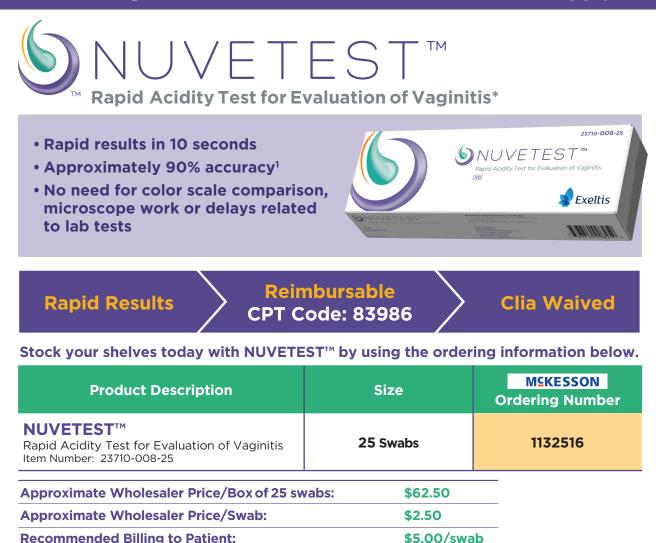

 Recommended Billing to Patient:
 \$5.00/swab

 To place an order or address guestions related to ordering, please contact McKesson at (855) 571-2100.

For first time customers, please set up an account using the following link: https://mms.mckesson.com/portal/login

Warnings and Precautions:

- Collect vaginal discharge from the anterior fornix or lateral vaginal wall of the mid vagina. Do not insert the NUVETEST[™] further than 5 cm (2") in the vagina, to avoid contact with the cervix mucus, where pH levels are known to be higher than normal vaginal pH.
- Do not use lubricants which alter vaginal acidity.
- If the patient is pregnant, the stain may indicate an amniotic fluid leakage.

To ensure valid results, do not use NUVETEST™ in any of the following conditions:

a) Less than 1 day before or the day after the patient's menstrual period;

- b) There are signs of menstruation or any vaginal bleeding;
- c) Less than 12 hours after sexual intercourse or use of vaginal products such as douching solutions or medications which alter vaginal acidity.

*Associated with Bacterial Vaginosis (BV), Trichomonas, and Vaginal Candidiasis

1. NUVETEST™ [prescribing information]. Exeltis USA, Inc.: Florham Park, NJ; 2018.



Please see full Information and Product Package Insert at NUVETEST.COM

NUVETEST[™] is a trademark of Exeltis Dermatology, LLC. © 2019 All rights reserved. Exeltis USA, Inc. EXP-19-0020 R00